

Figure 1

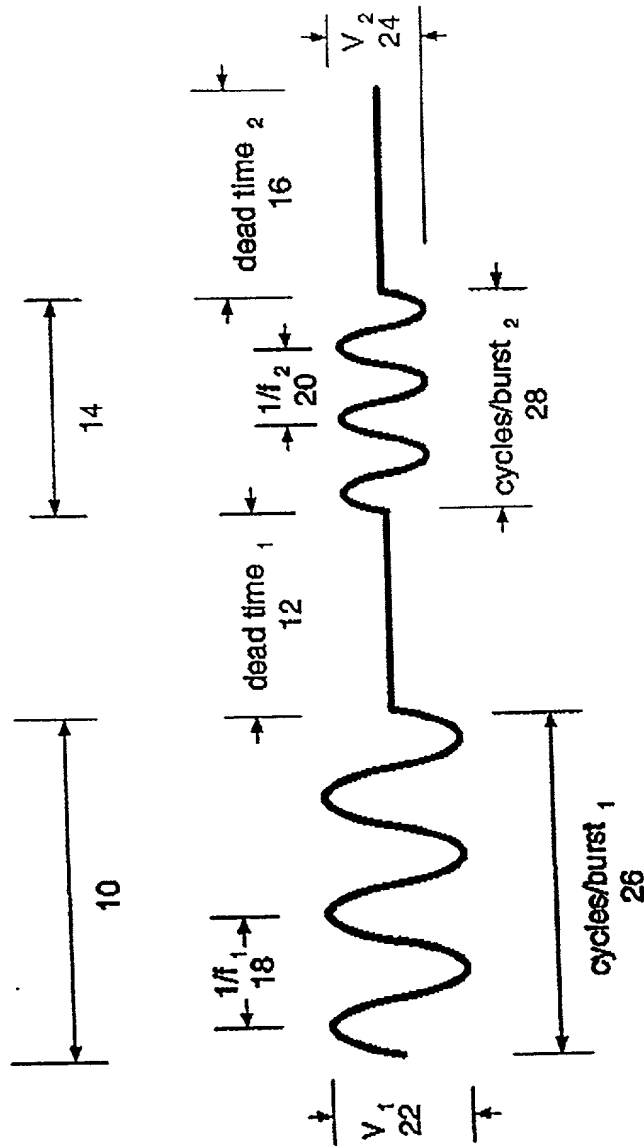


Figure 2






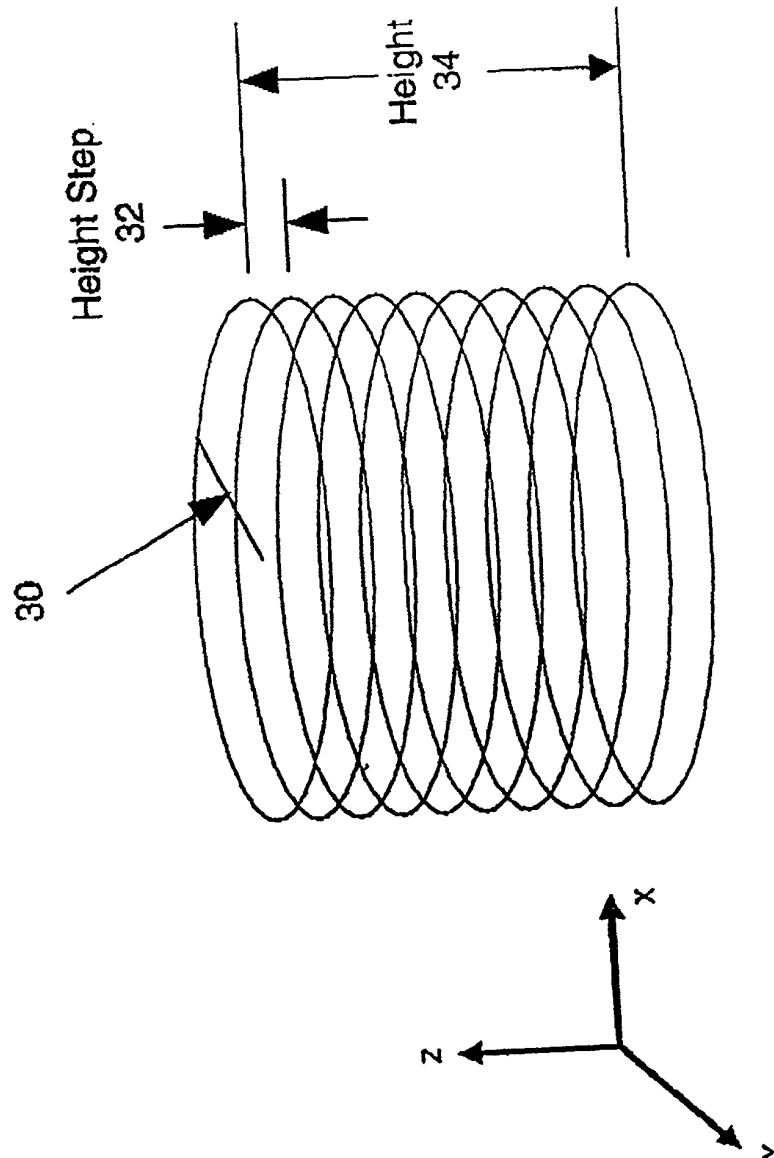


Figure 3




post-treatment  
transfer

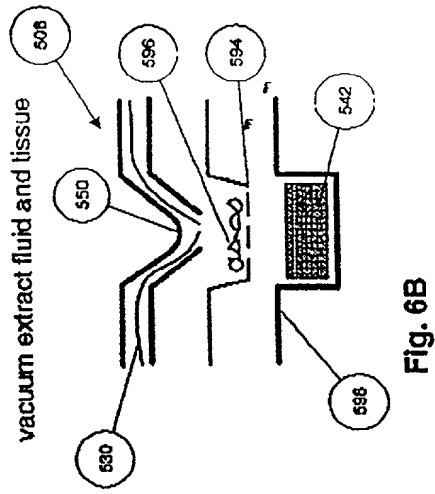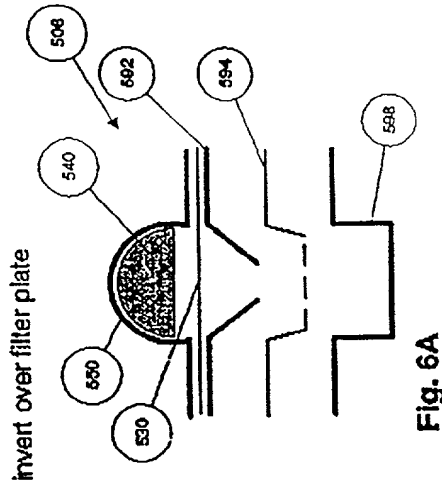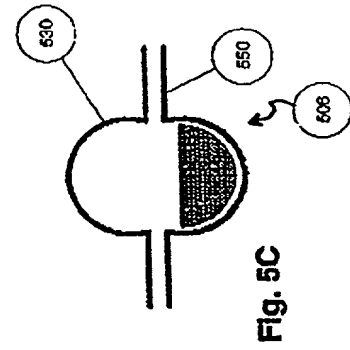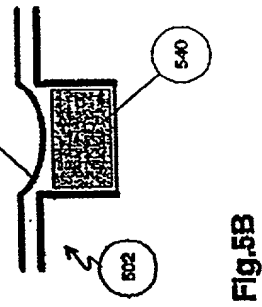

pre-treatment  
assembly

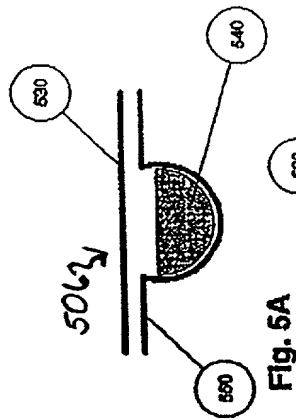

treatment  
vessels

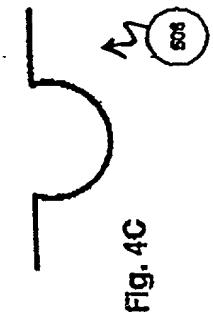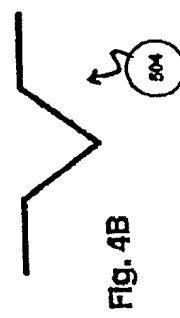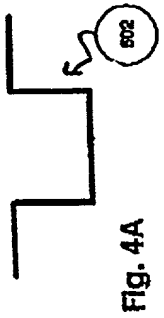

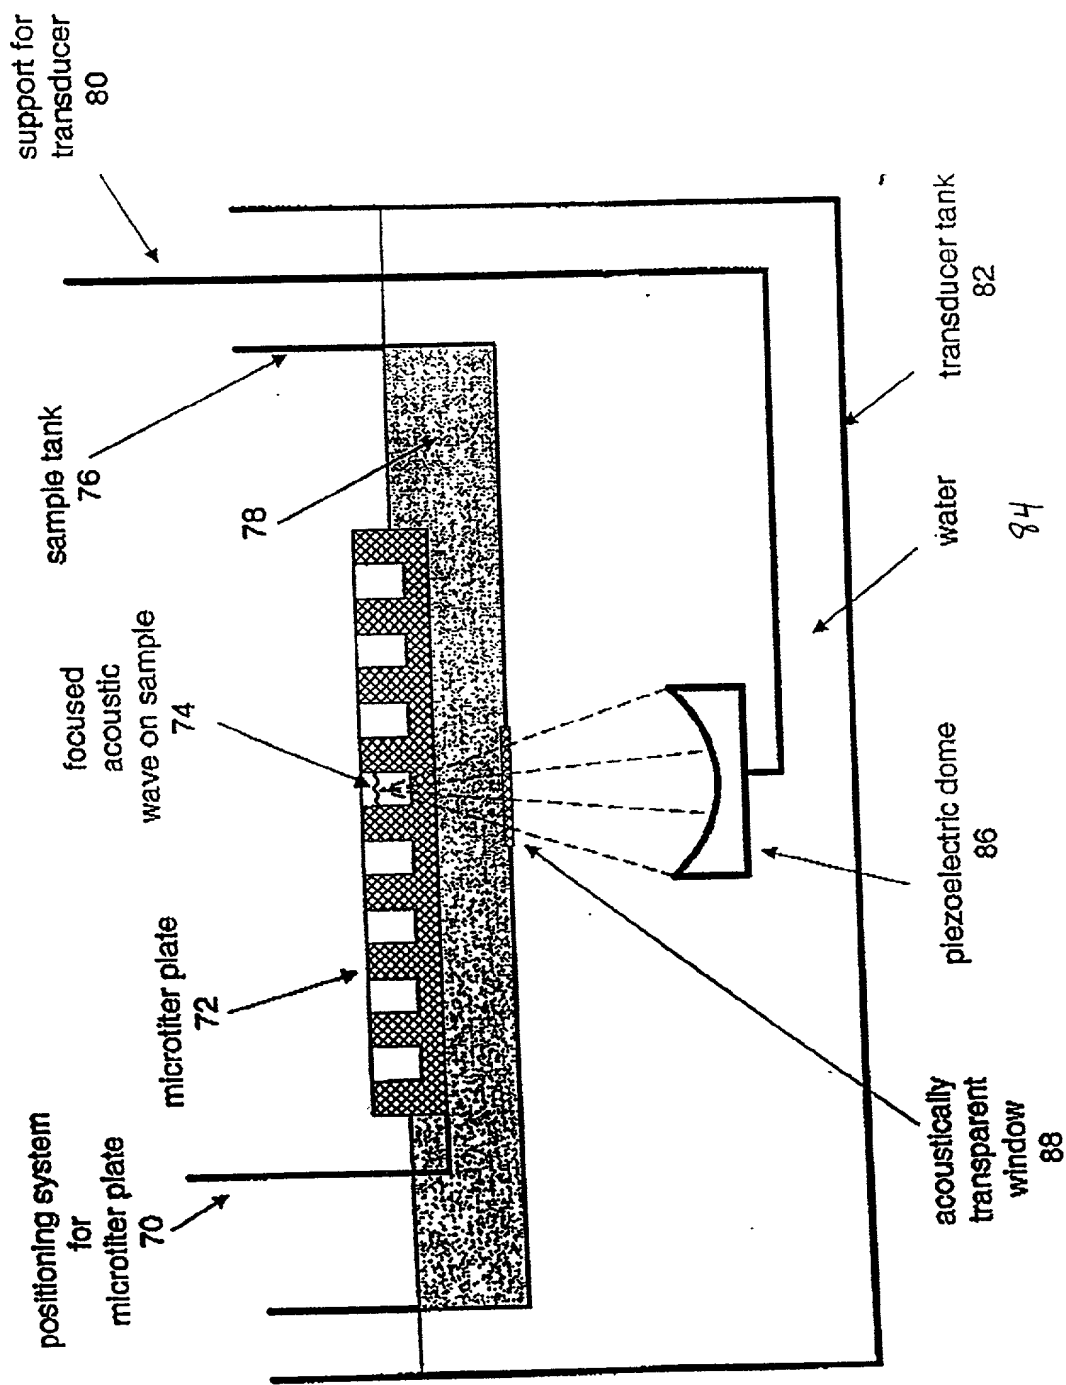


Figure 7

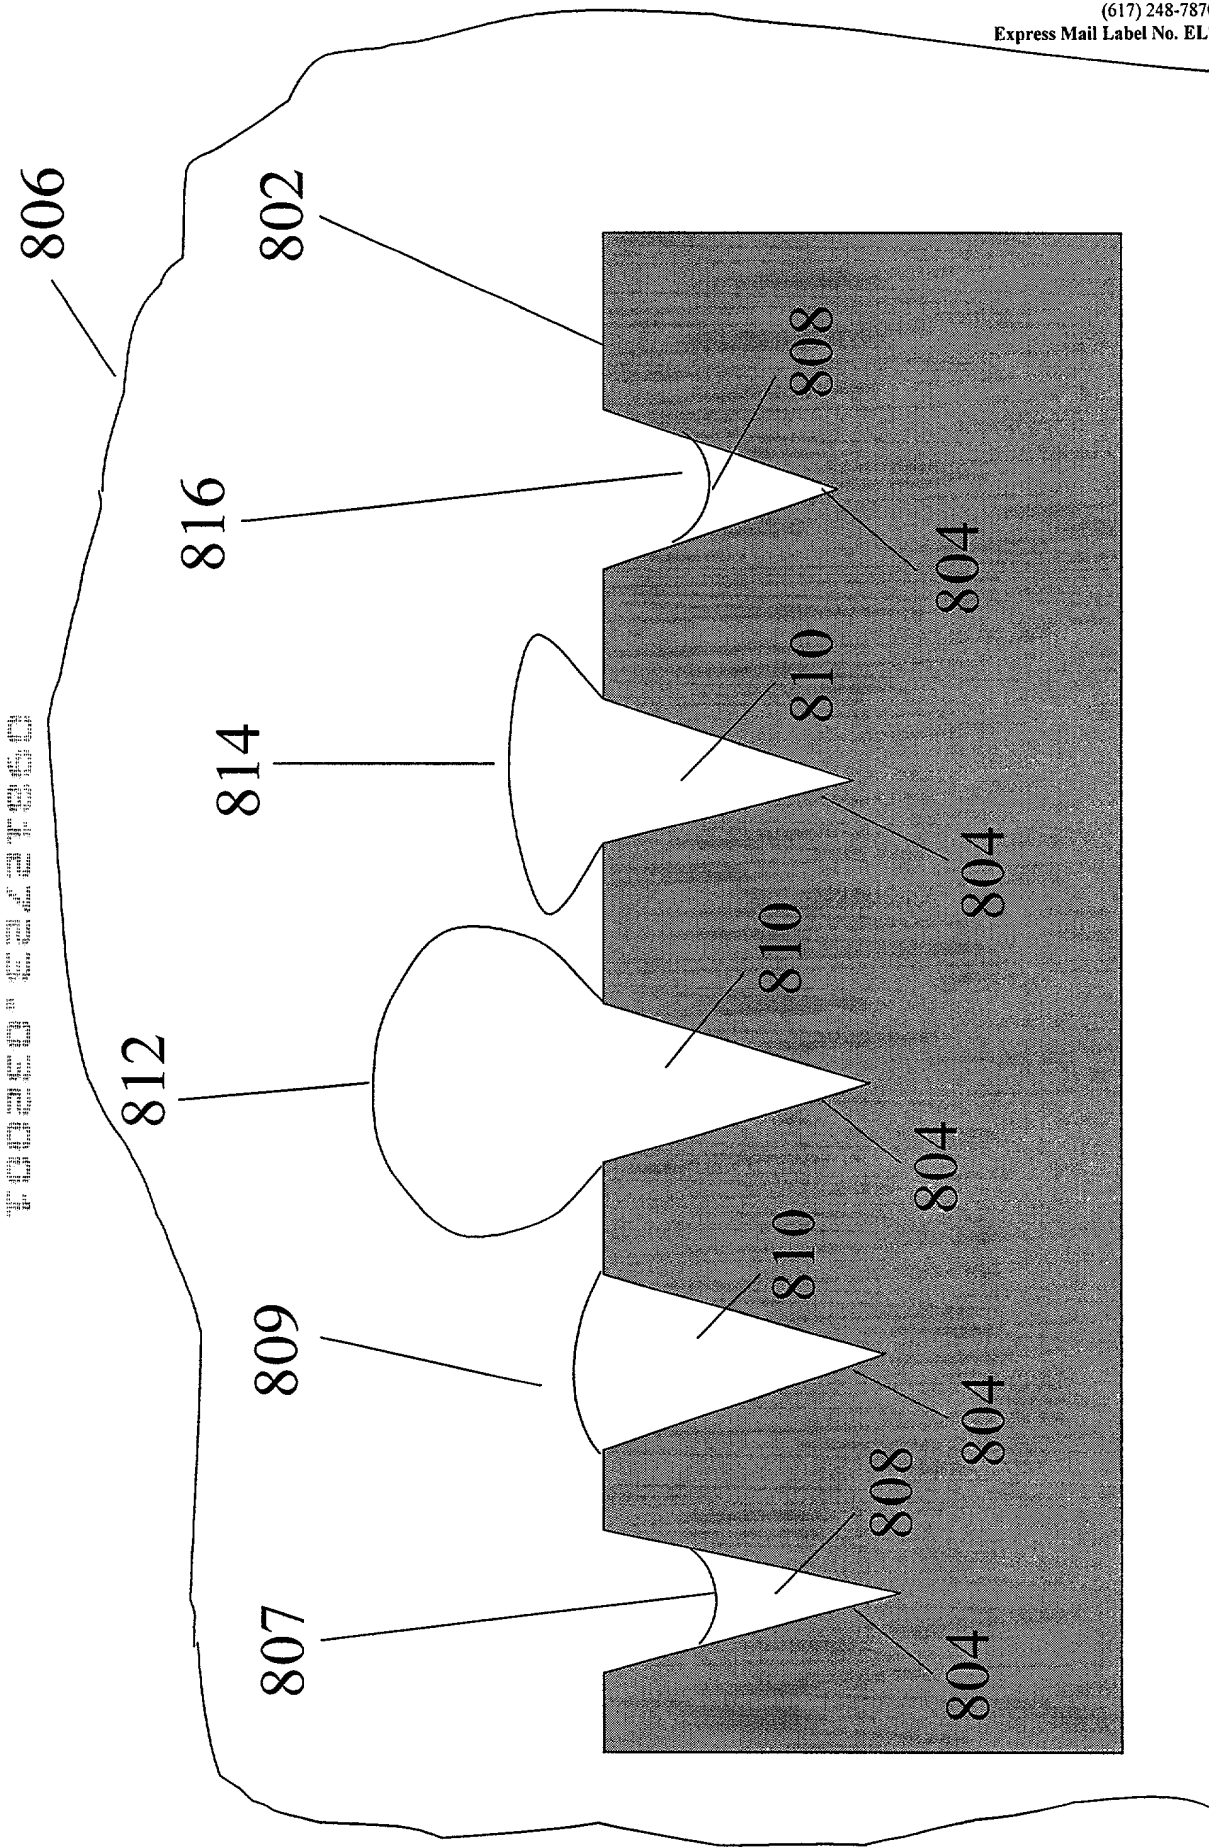


Figure 8  
 2046645

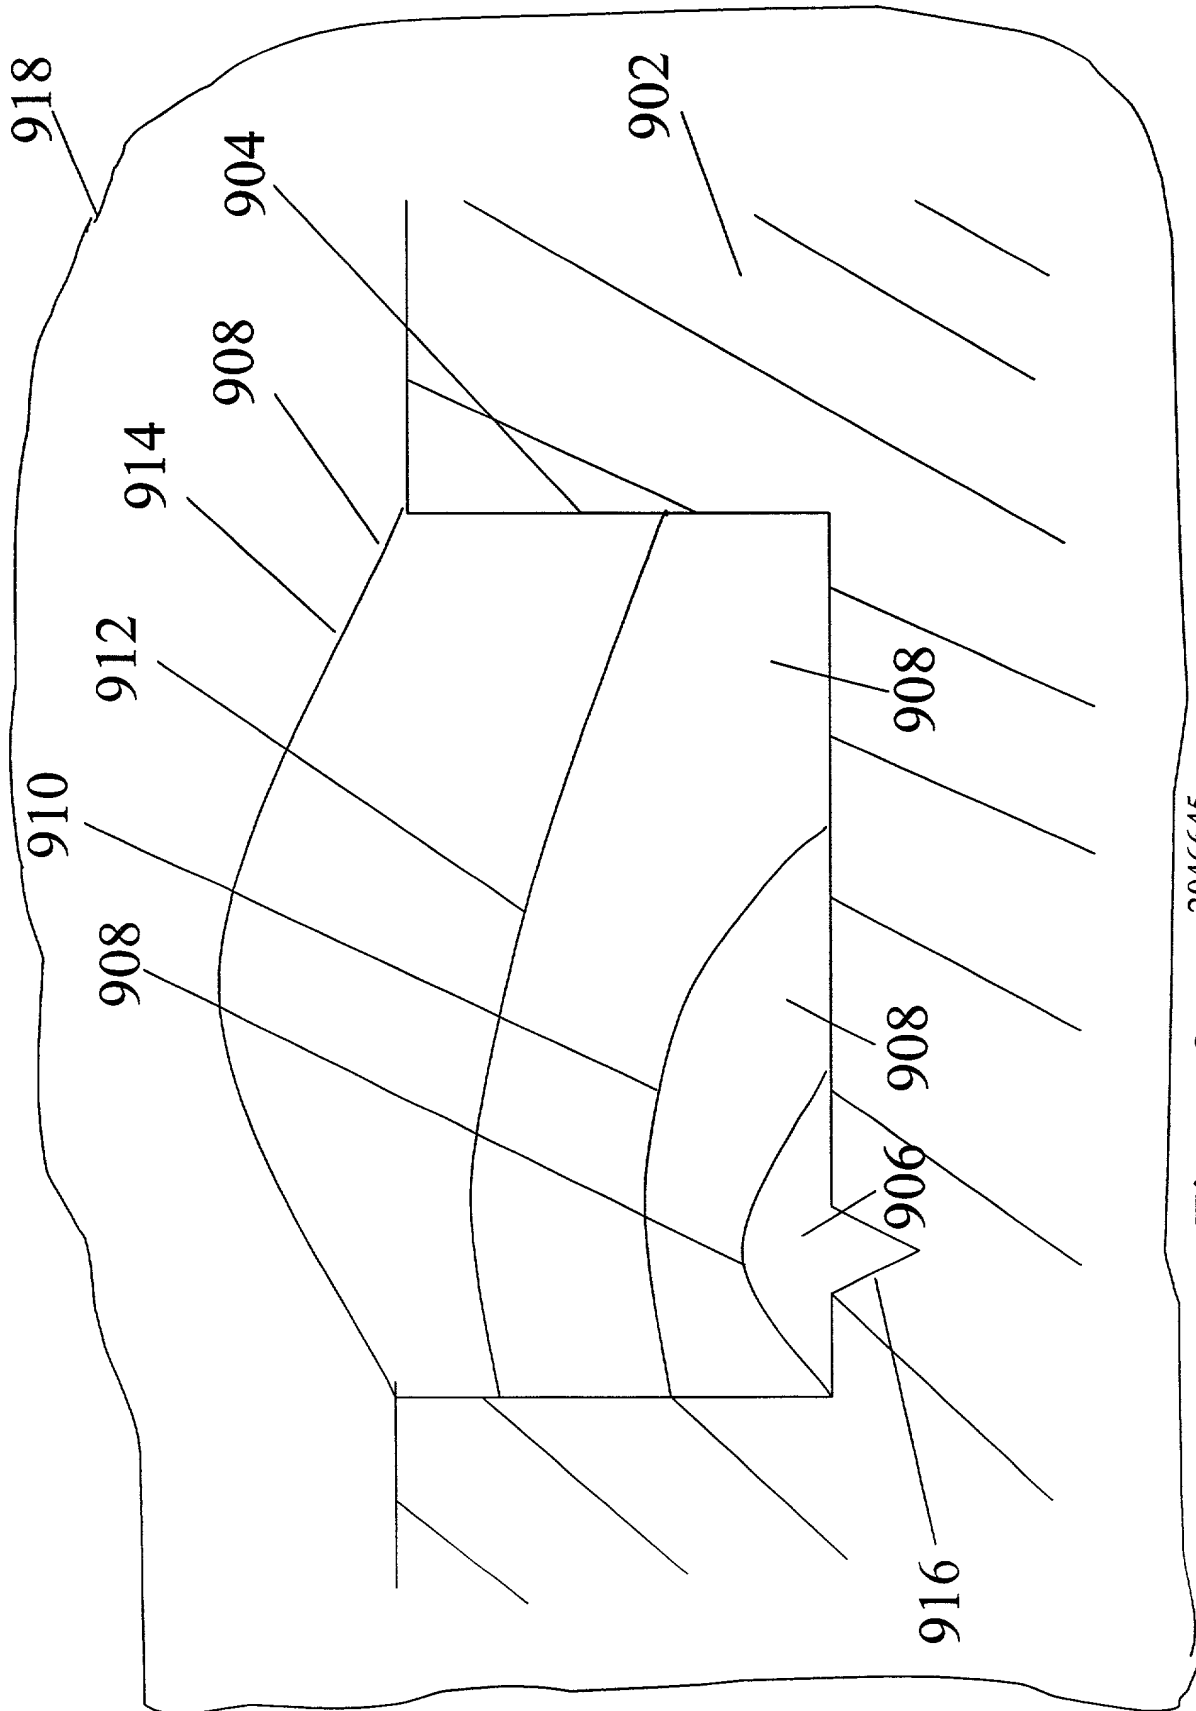


Figure 9

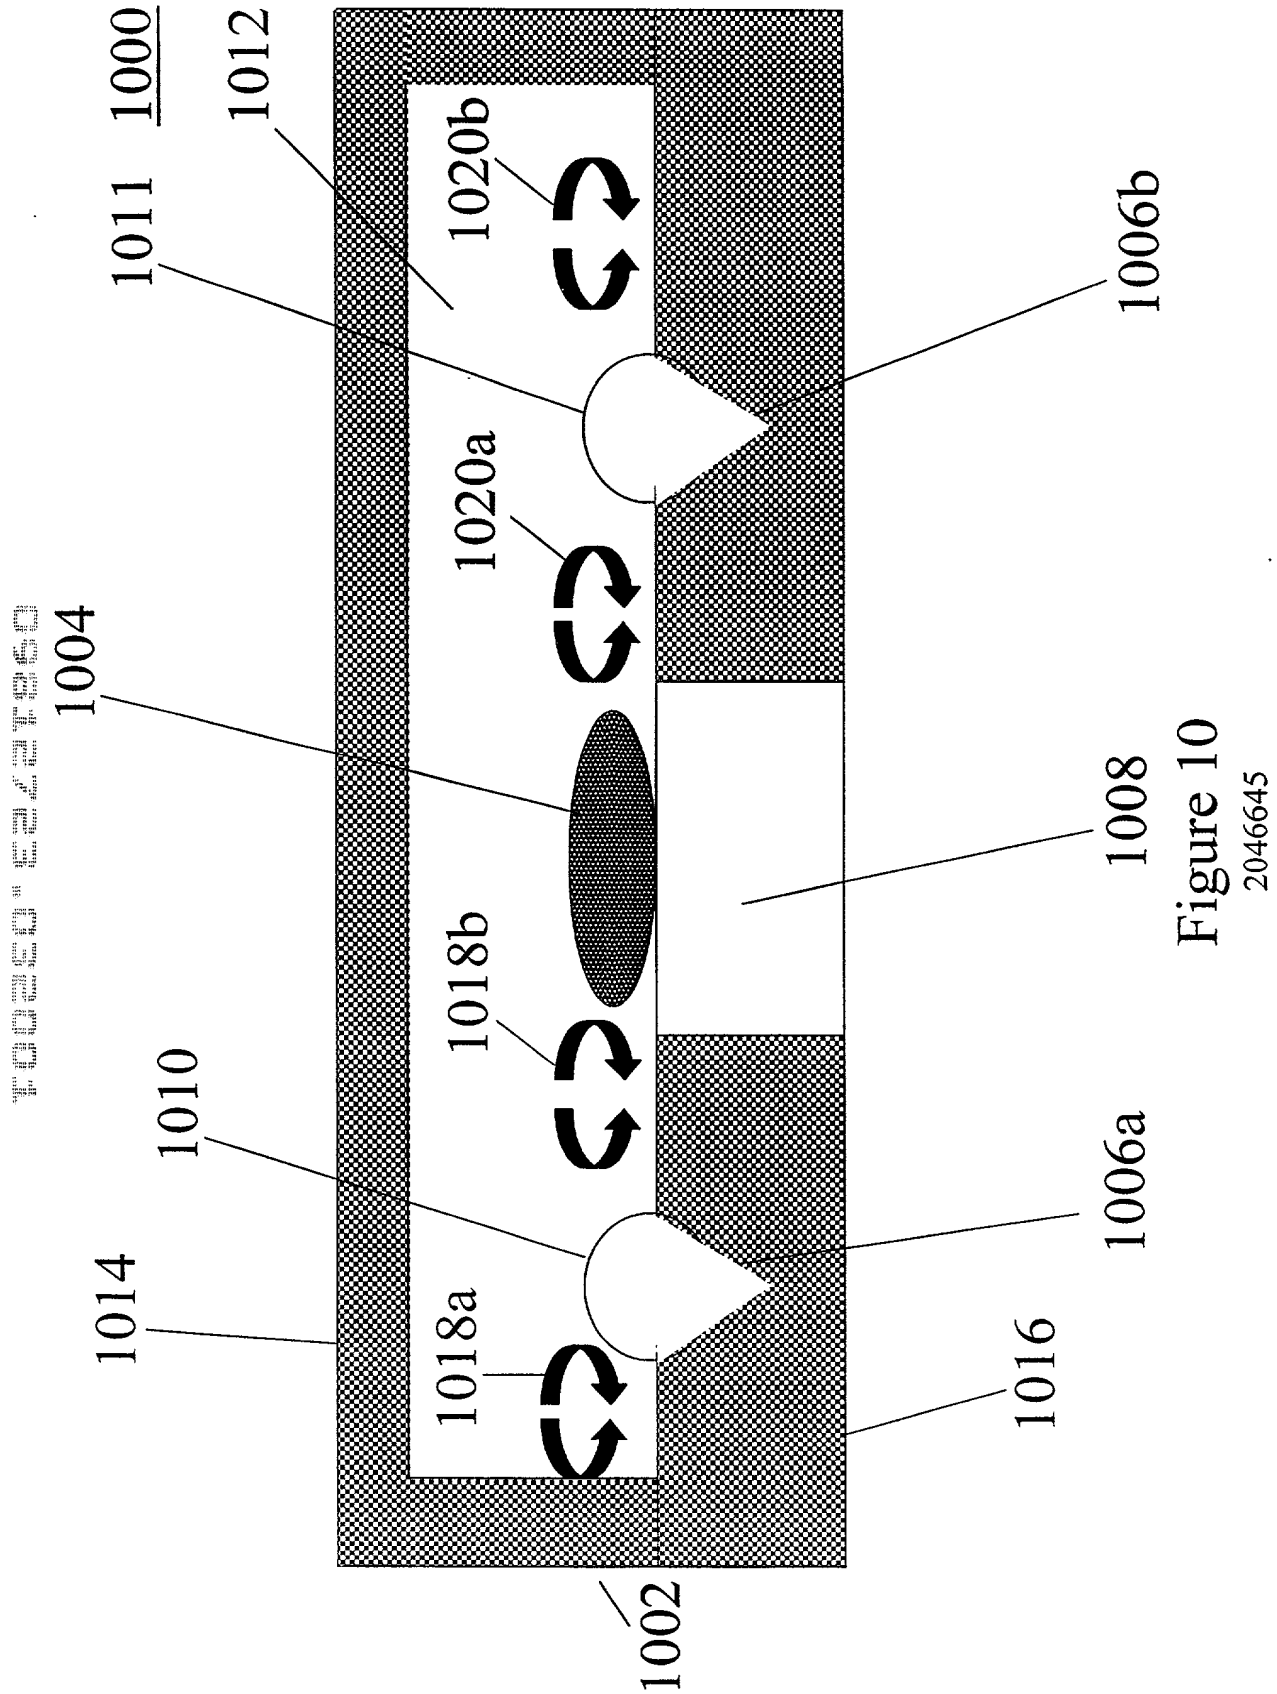


Figure 10  
2046645



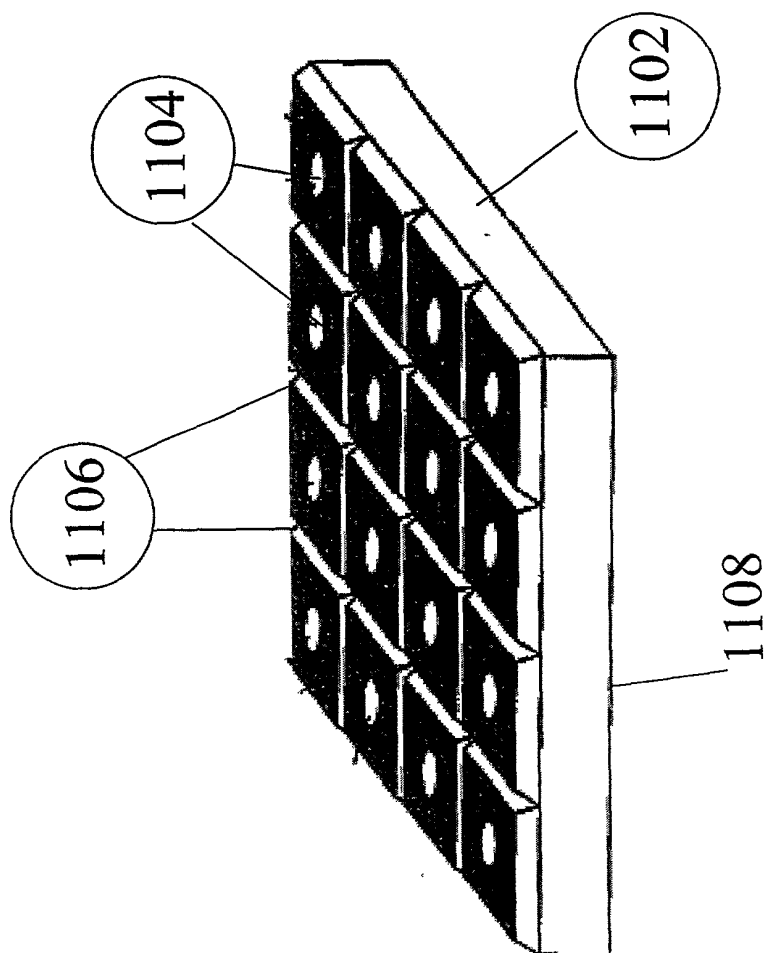


Figure 11

2046645

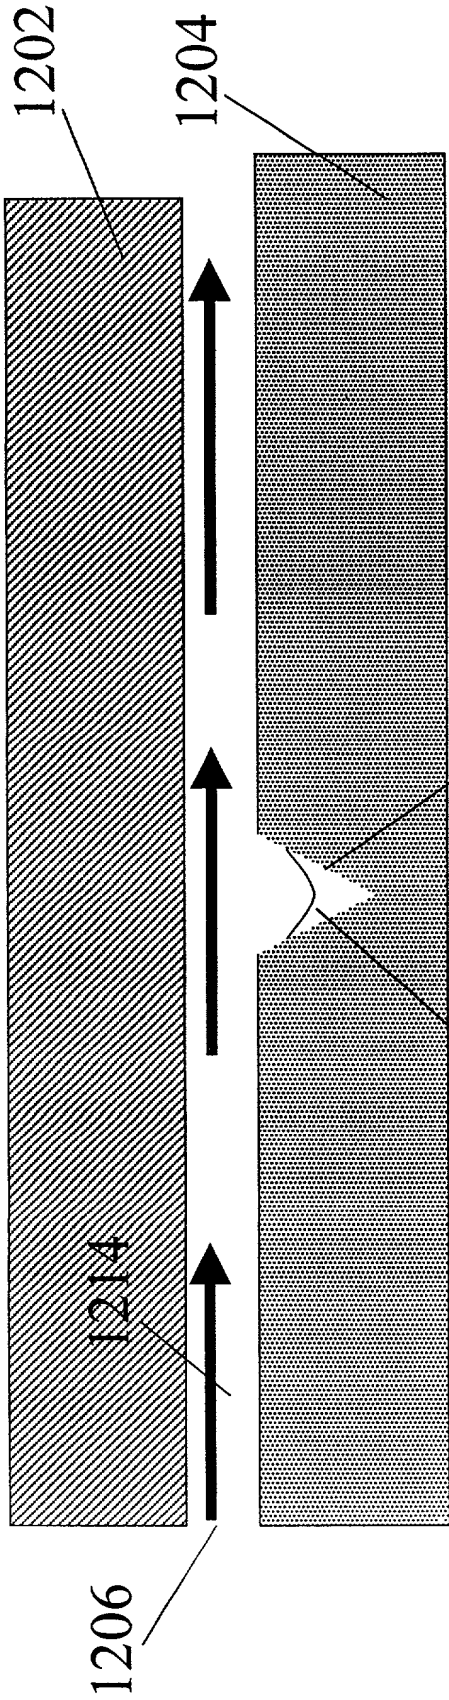


Figure 12A 1208 1210 1212

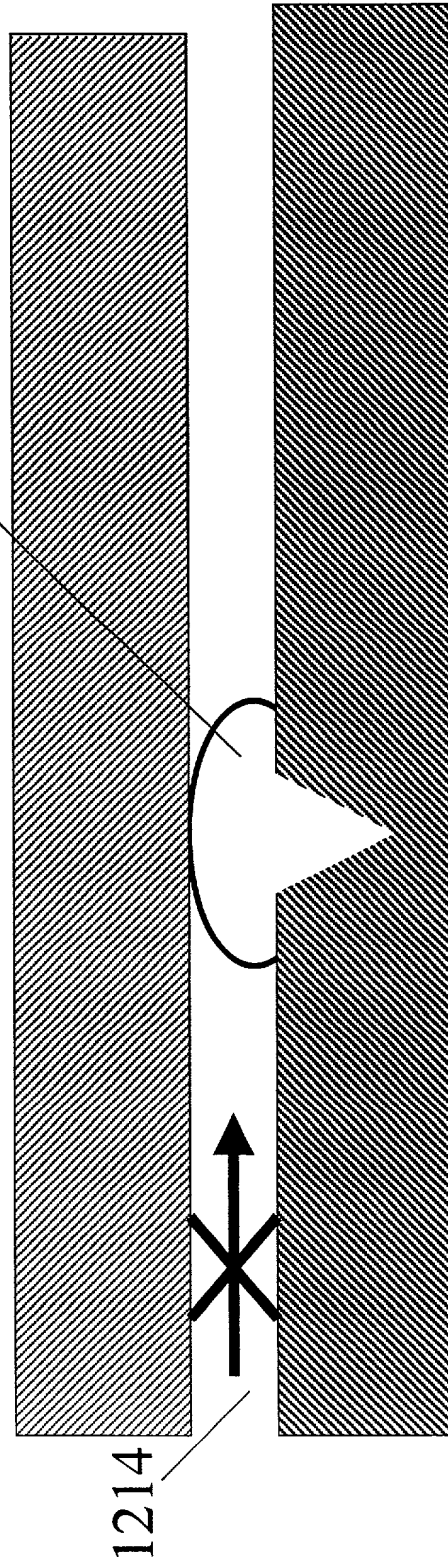
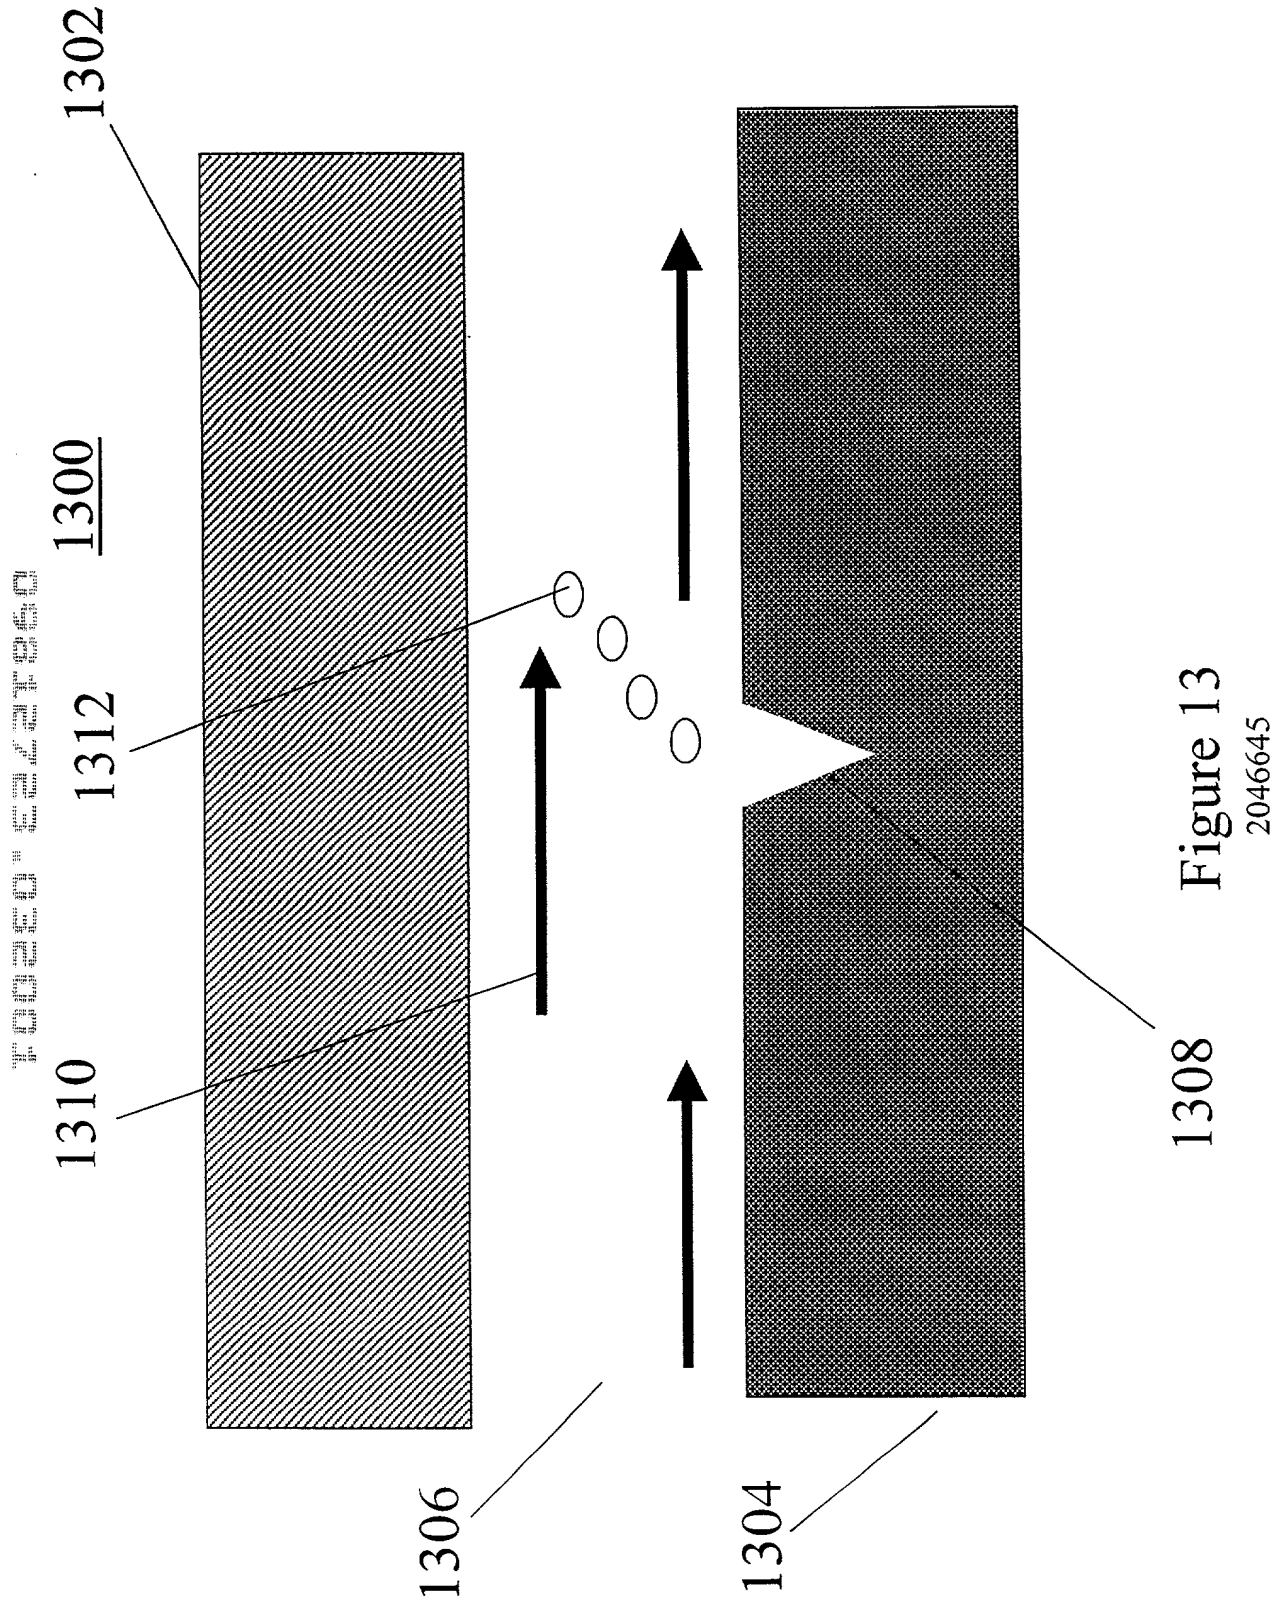


Figure 12B 2046645



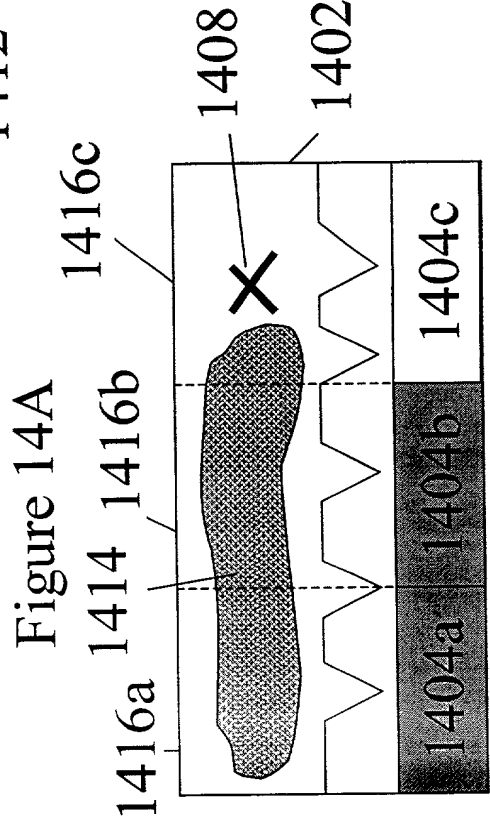
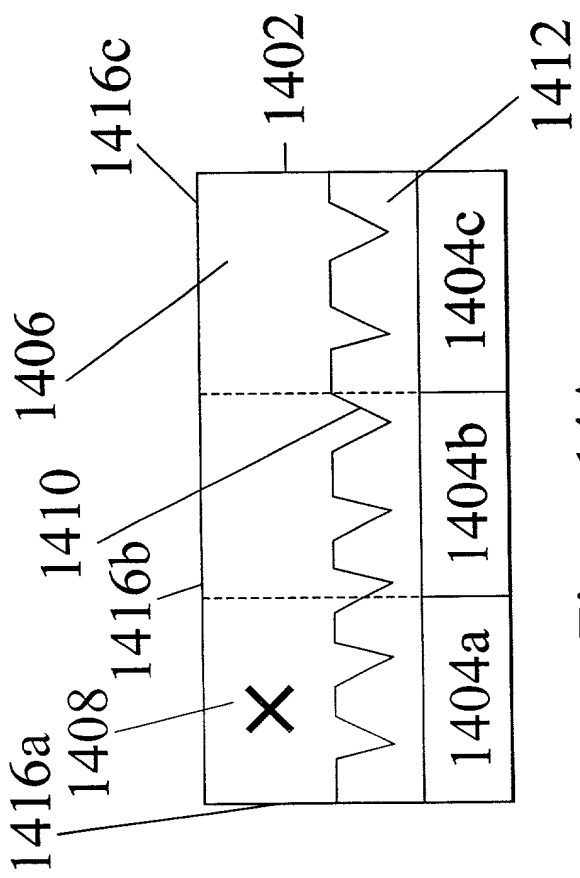


Figure 14C

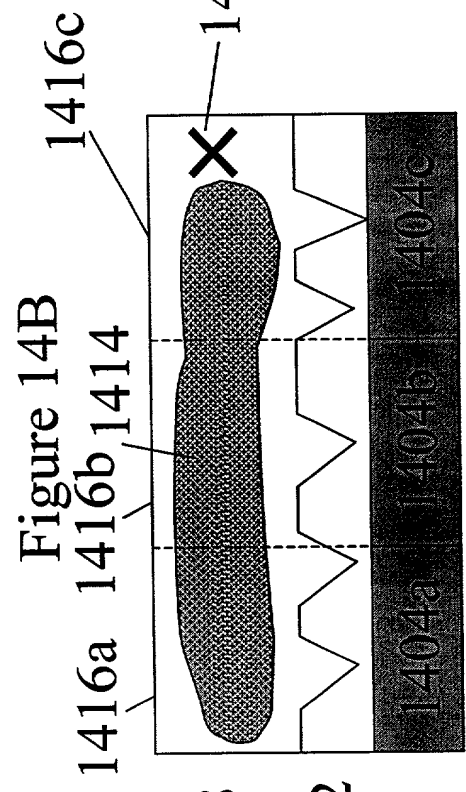
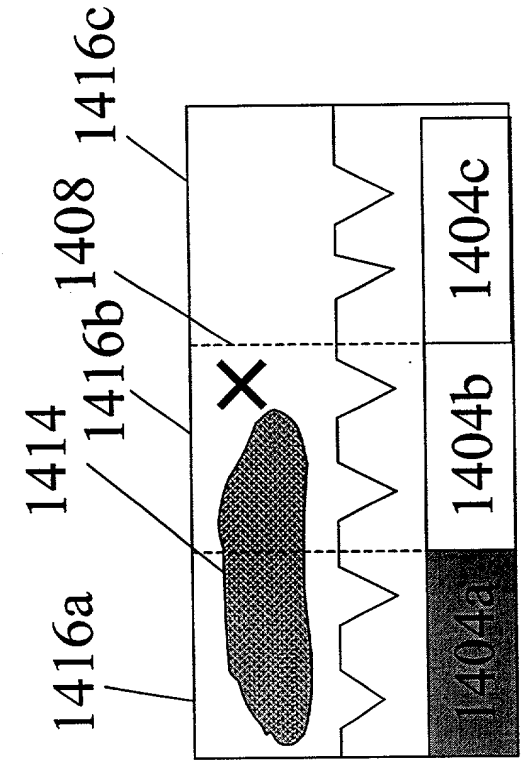


Figure 14D

2046645

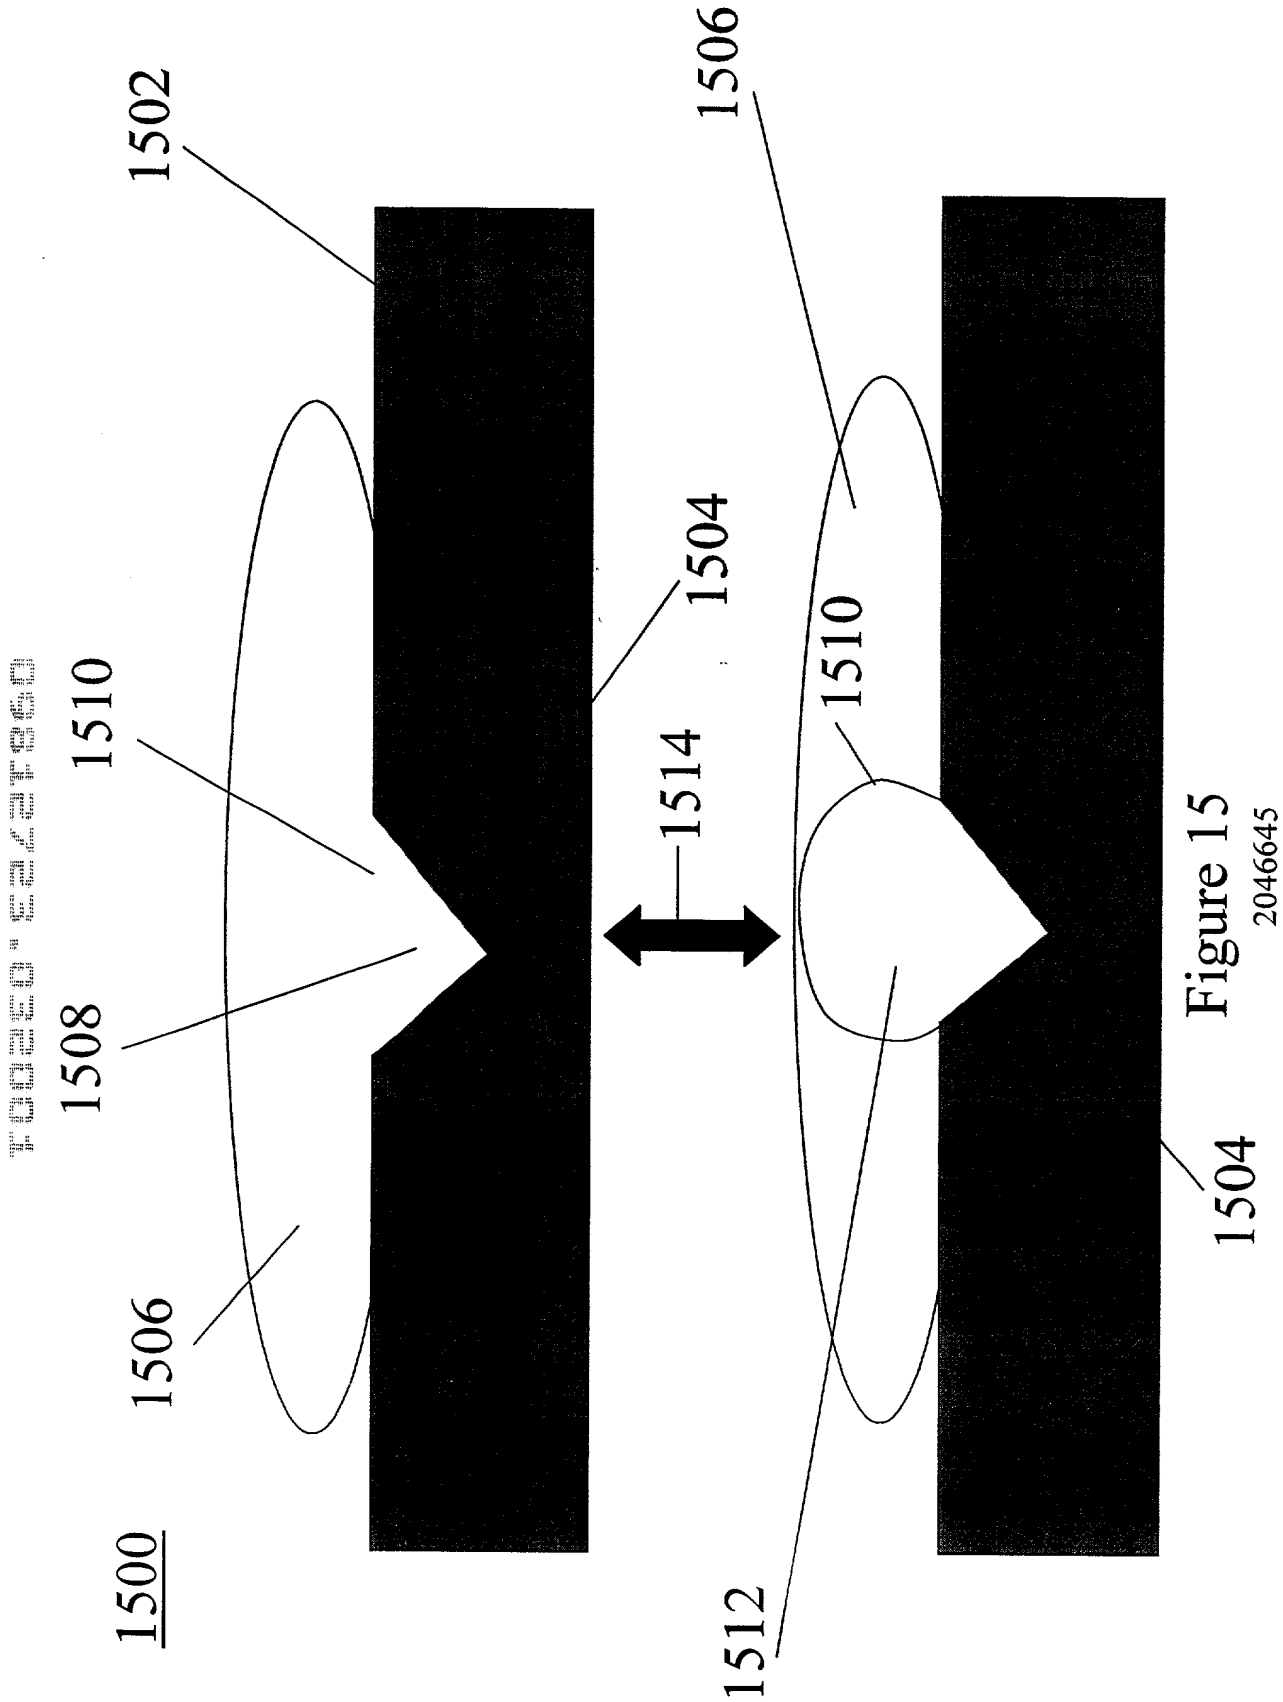


Figure 15  
2046645

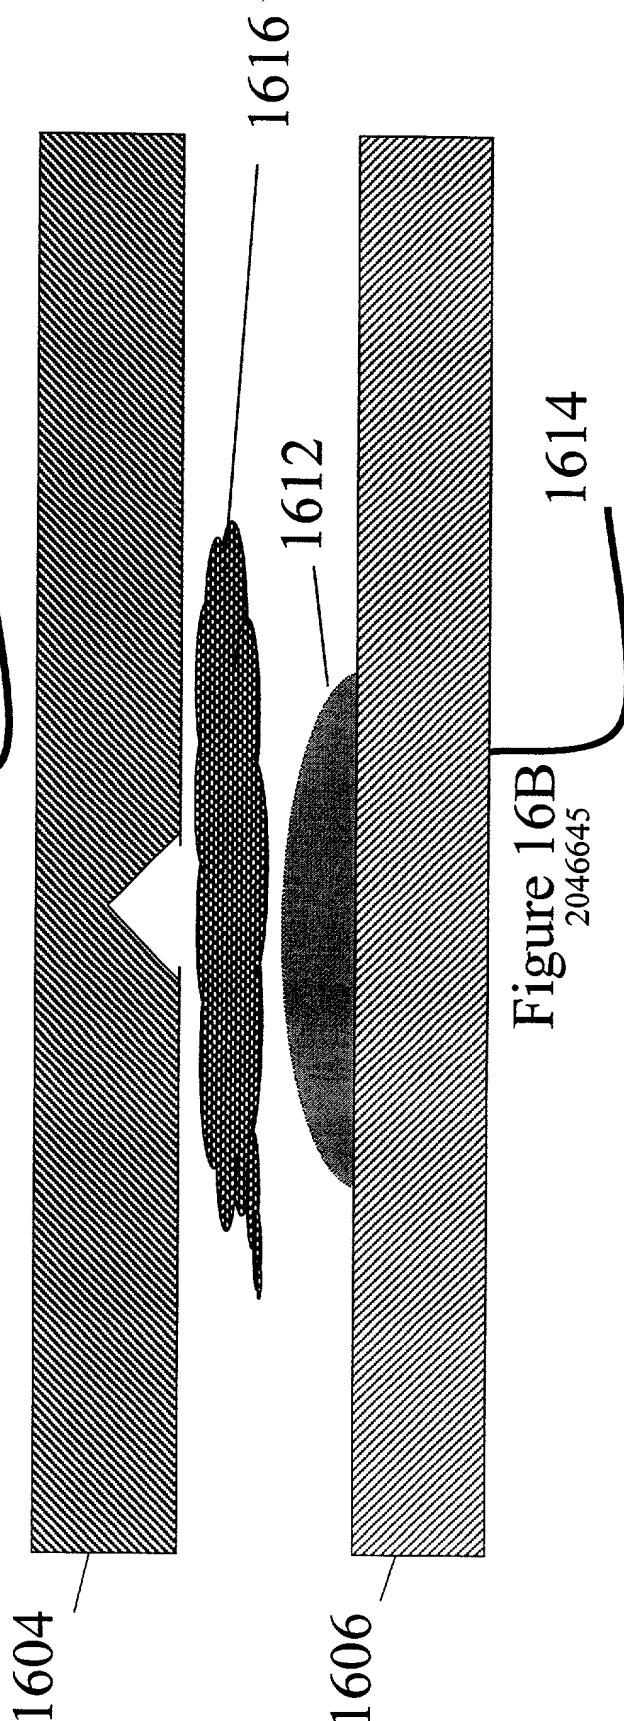
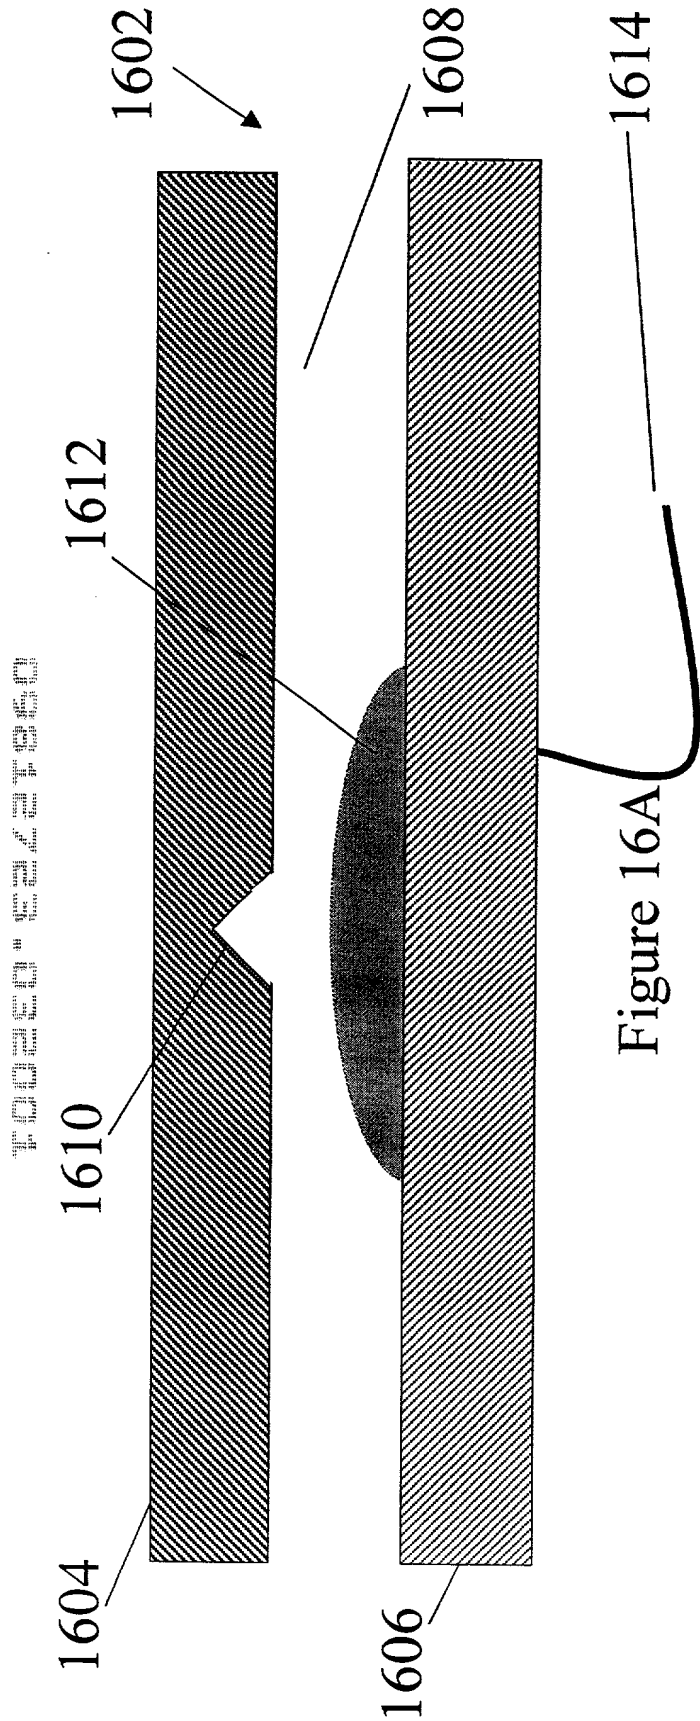


FIG. 17

1700

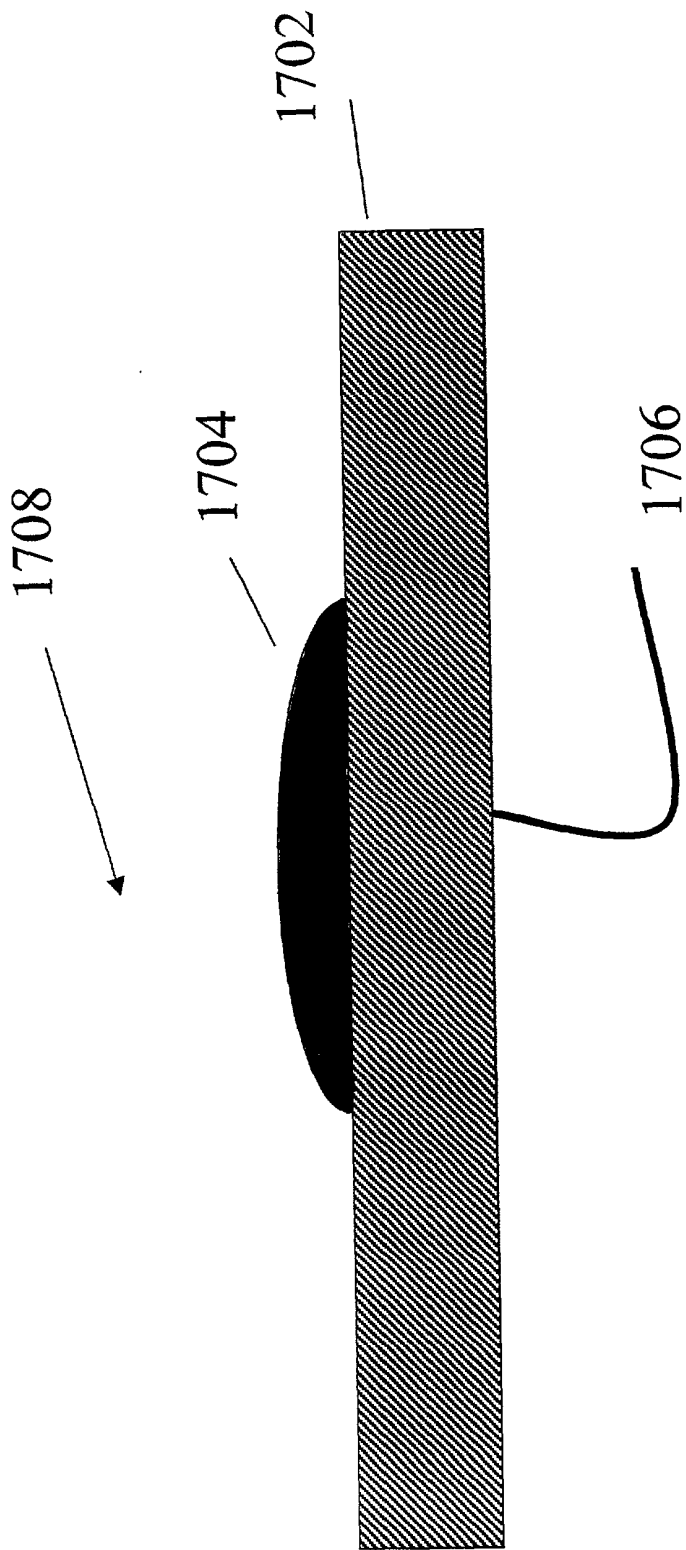


Figure 17

2046645

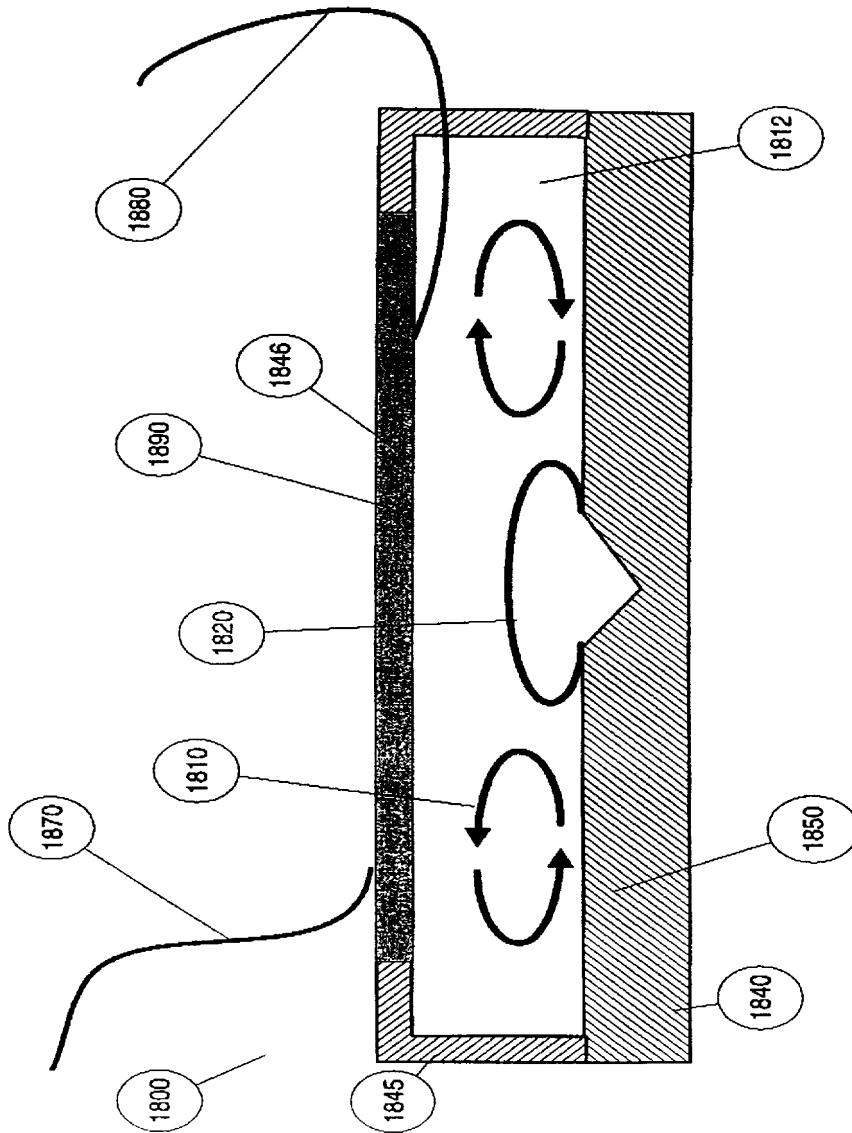


FIGURE EIGHTEEN